



Manufacturer	Cochlear
Processor	Nucleus 7 (CP1000)
Manufacturer website	https://cochlear.com/
Cochlear implant clinic / location	
Audiologist name / contact information	

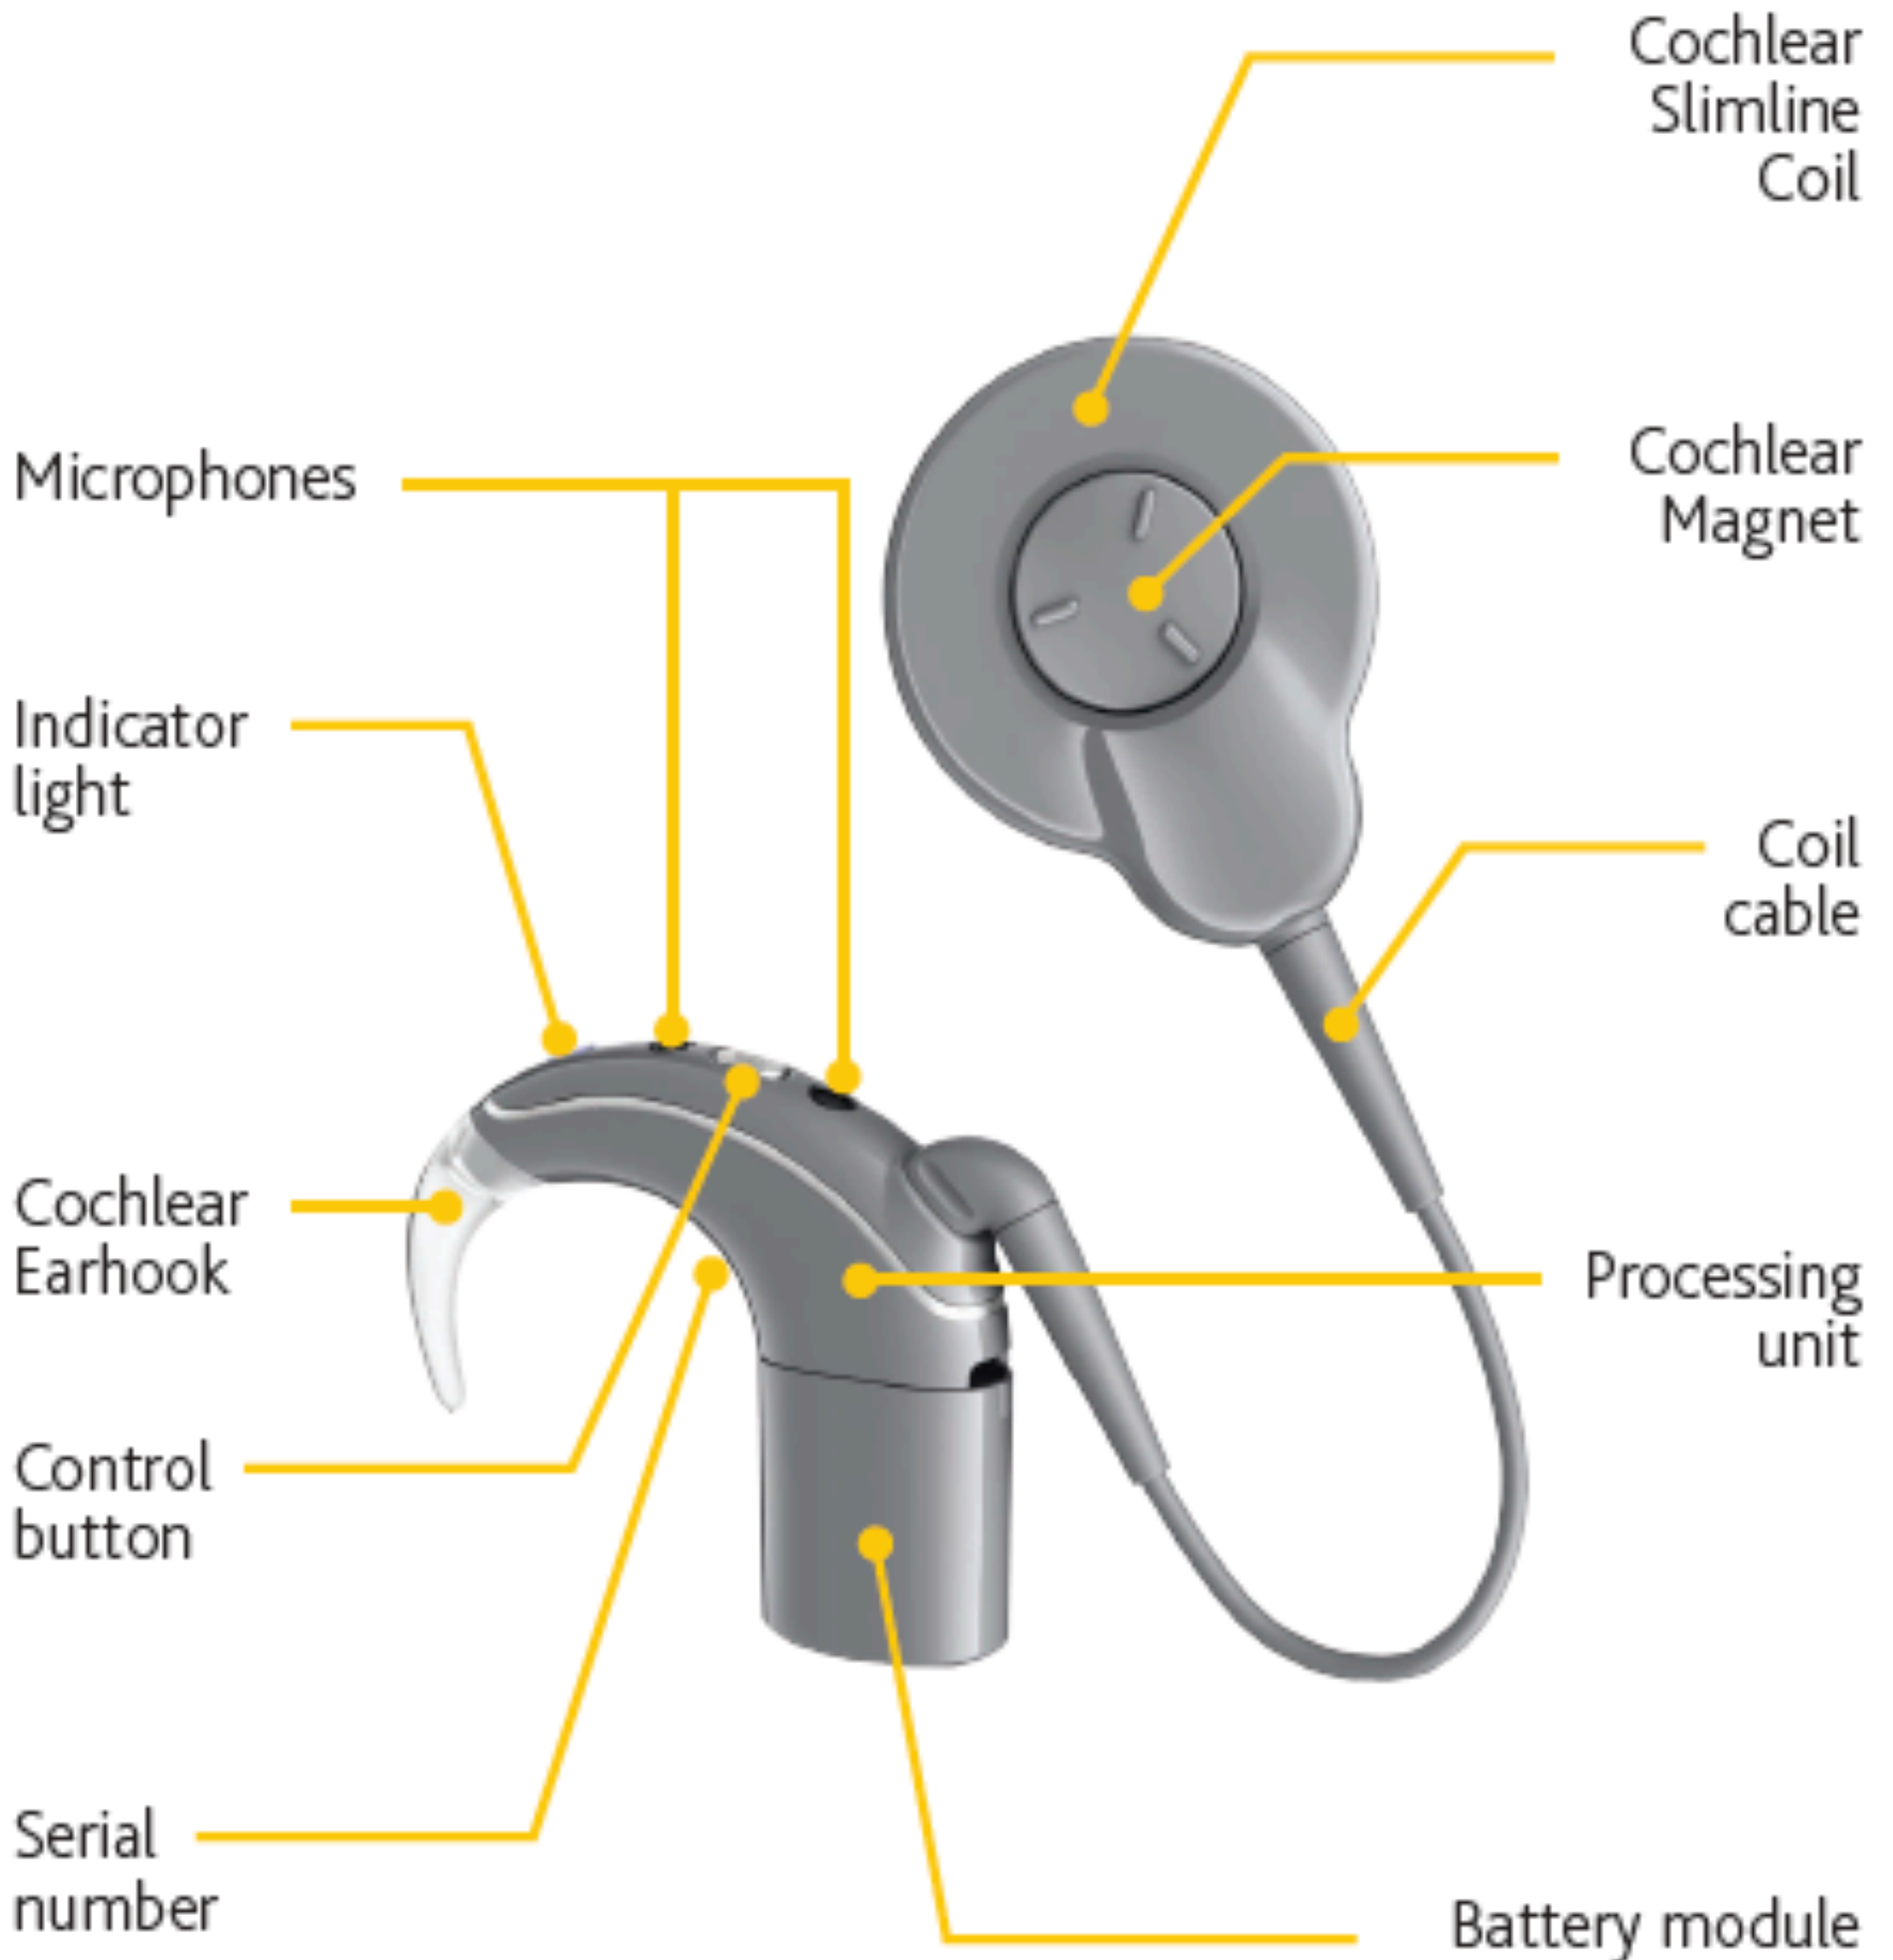


Manufacturer	Cochlear
Processor	Kanso (CP950)
Manufacturer website	https://cochlear.com/
Cochlear implant clinic / location	
Audiologist name / contact information	

Front

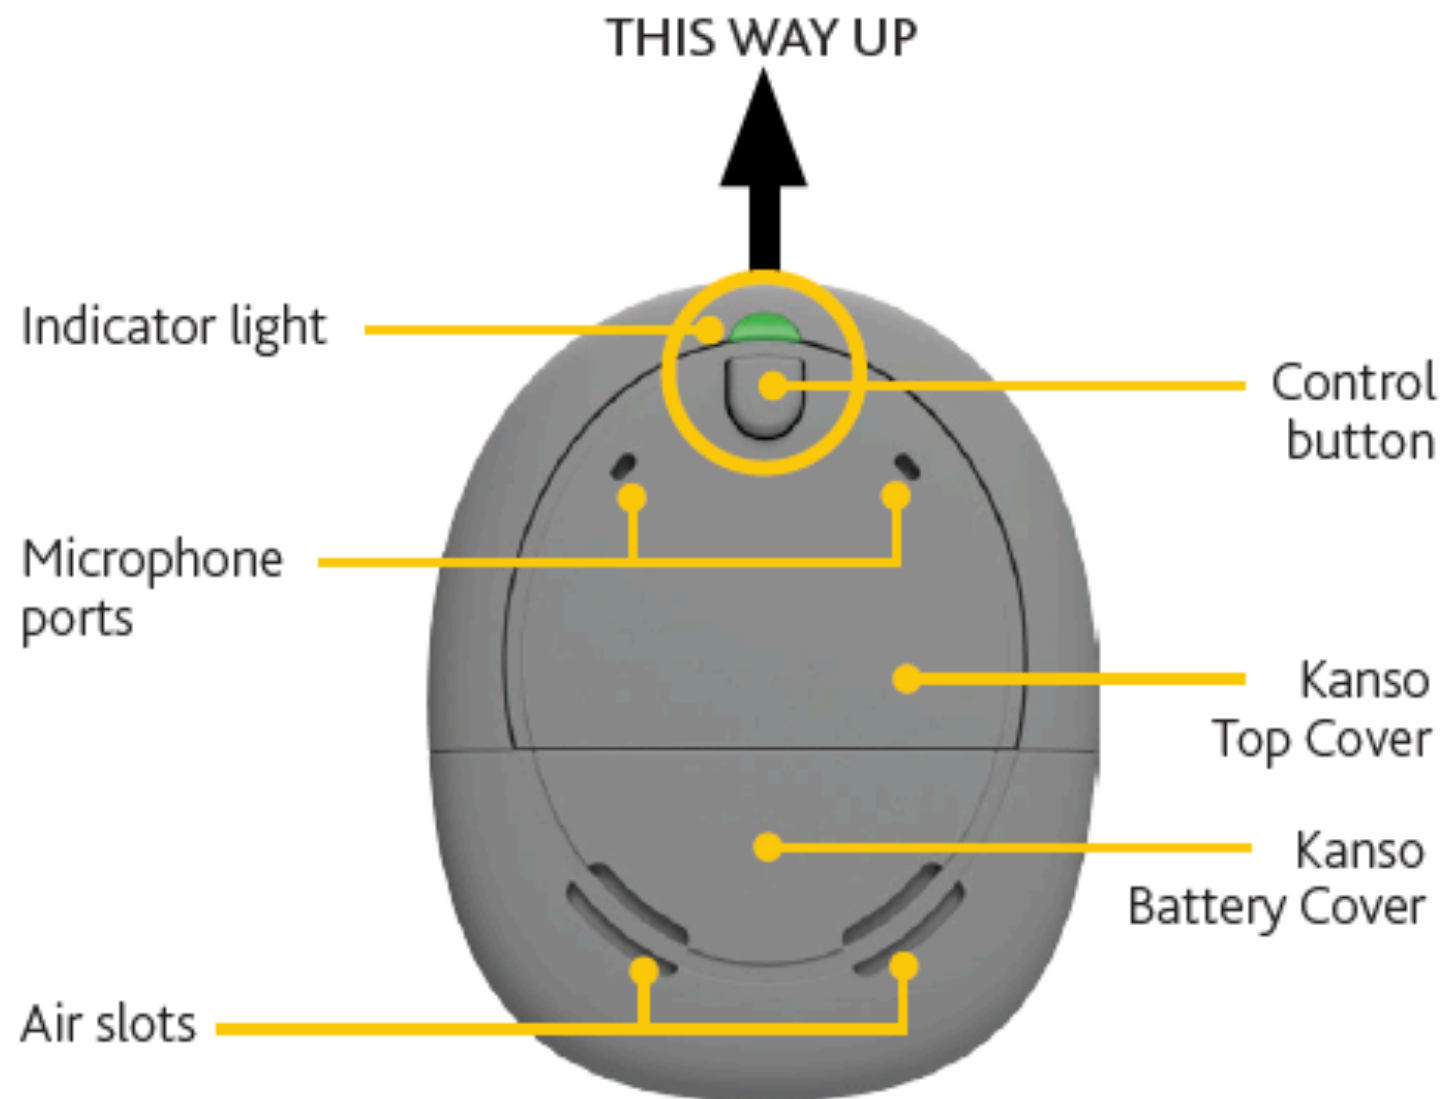

Back

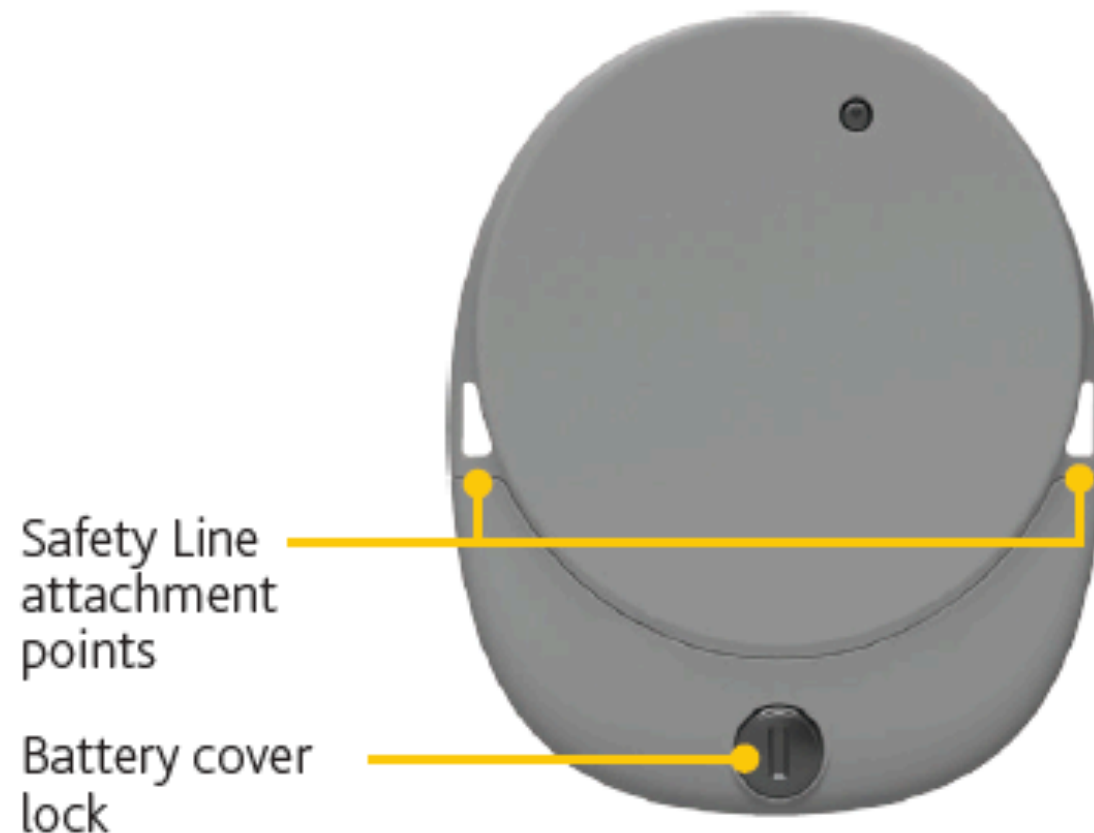

Manufacturer	Cochlear
Processor	Nucleus 6 (CP910 – standard rechargeable / CP920 – compact rechargeable)
Manufacturer website	https://cochlear.com/
Cochlear implant clinic / location	
Audiologist name / contact information	



Manufacturer	Cochlear
Processor	Nucleus 5 (CP810)
Manufacturer website	https://cochlear.com/
Cochlear implant clinic / location	
Audiologist name / contact information	



1. Coil
2. Coil magnet
3. Coil cable
4. Lower button
5. Microphones
6. Upper button
7. Indicator light
8. Earhook
9. Processing unit
10. Battery module
11. Accessory socket cover